



REC'D 22 JUN 2004

WIPO

PCT

# Kongeriget Danmark

Patent application No.: PA 2003 00813

Date of filing: 30 May 2003

Applicant:  
(Name and address) Alsensa ApS  
c/o Helena Bøttkjær  
Adolfsvej 56  
DK-2820 Gentofte  
Denmark

Title: Allergy tester

IPC: -

This is to certify that the attached documents are exact copies of the above mentioned patent application as originally filed.



**PRIORITY DOCUMENT**  
SUBMITTED OR TRANSMITTED IN  
COMPLIANCE WITH  
RULE 17.1(a) OR (b)

Patent- og Varemærkestyrelsen  
Økonomi- og Erhvervsministeriet

18 June 2004

*Susanne Morsing*  
Susanne Morsing

**BEST AVAILABLE COPY**

P 780 DK00

Modtaget

30 MAJ 2003

PVS

1

**Allergy tester**

The present invention relates to a device for delivering a medicament or a diagnostic agent to the skin or mucosa of an animal such as a human being, wherein the chamber filled with the medicament or the diagnostic agent is separate from the housing with a rod capable of transferring the medicament or the diagnostic agent to the animal. In particular the invention relates to a device for delivering allergens in allergy tests.

**Background**

In recent years, allergies have become an increasing problem especially in the Western World. Therefore, the need for being able to diagnose such diseases quickly, securely and reproducibly is growing steadily.

Conventionally, allergies are diagnosed by manually applying a number of different allergen solutions on the palm side of the patient's forearm. After this, an injection needle is pricked through the individual drops and about 1 mm into the skin so that a cavity is formed for absorbing some of the solution.

If the person is allergic to an allergen solution, the skin will after 10 to 15 minutes become red and swollen around the injection spot to an extent that depends on the quantity or the concentration of the solution that can be absorbed by the cavity. The degree of the allergic reaction can be given as a function of the extent of the swelling.

It is very difficult to dose the solution quantity with great accuracy, however, as the insertion depth of the needle and thereby the cubic capacity of the cavity depends solely on the operator's routine and skill.

With the above conventional method, the degree of the allergic reaction can therefore not be estimated with the wanted accuracy and reproducibility.

As various allergen extracts are often used at tests of an allergic reaction, there is moreover an added risk of confusing the test solutions. Furthermore, the solutions

are placed directly on the skin, which opens up the possibility of contamination with allergizing agents that might give a false positive response. By using this open handling of the allergen extracts, there is furthermore a risk of the operator becoming sensitized to one of the respective allergen extracts.

5

An additional problem of the conventional method is the risk of infection which is present to the operator in that the injection needle remains unprotected after use. U.S. Pat. No. 5,099,857 discloses a construction with a movable injection needle and a sealed capsule containing an allergen solution. At injection, the needle will rupture the capsule, and the solution will therefore run out and form a drop on the skin, after which the needle via the drop will penetrate the skin in the same way as mentioned above. Also in this case, the estimate of the possible skin reaction will be inaccurate. Thus, there is a need for improvements in such devices.

10

15

### Summary

The present invention provides a solution to prior art problems by providing a device for delivering a medicament or a diagnostic agent to the skin or mucosa of an animal, said device comprising

20

at least one rod house and at least one separate chamber house, wherein said chamber house is capable of being connected to the rod house,

25

wherein the rod house comprises at least one housing, said at least one housing having a distal end and a proximal end, and at least one rod, said rod having a distal end and at least one proximal end, and said rod being slidably arranged in the housing, said rod being capable of being activated by being pushed towards the proximal end of the housing, and

30

wherein the chamber house comprises at least one chamber, a first wall of said chamber being a first sealing and a second wall of said chamber being a second sealing, said first sealing and said second sealing being arranged so that an axis through said chamber may intersect both sealings, and said chamber comprising said medicament or said diagnostic agent.

35

5 By the device according to the invention, the medicament or diagnostic agent is enclosed in the chamber until activation of the rod, whereby the risk of contamination is eliminated. Furthermore, in particular when testing for allergy, it is of importance that the various allergens are not mixed, a problem that is reduced with the present invention. Also, the device presents a solution to storage problems, since the chamber house may be stored separate from the rod house, and the chamber is the only part needing refrigerated storage.

10 The device according to the invention provides delivery of the medicament or diagnostic agent easily, quickly, with less pain and greater accuracy and reproducibility than prior art devices.

15 In another aspect the invention relates to a method for delivering a sufficient amount of medicament or diagnostic agent to an animal in need thereof, comprising

- arranging a device as defined above, wherein the chamber house comprising the medicament or diagnostic agent is connected to the rod house, adjacent the skin or mucosa of said animal,
- 20 - activating the rod of the device, thereby delivering said medicament or diagnostic agent to said animal.

In particular the method is suitable for allergy tests.

25 Furthermore, the invention relates to a separate chamber house for being connected to a rod house as defined above, wherein the chamber house comprises a chamber, a first wall of said chamber being a first sealing and a second wall of said chamber being a second sealing, said first sealing and said second sealing being arranged so that an axis through said chamber may intersect both sealings, and said chamber comprising a medicament or a diagnostic agent.

30 Also, the invention relates to a separate rod house comprising at least one housing, said at least one housing having a distal end and a proximal end, and at least one rod, said rod having a distal end and at least one proximal end, and said rod being slidably arranged in the housing, said rod being capable of being activated by being

35

4

pushed towards the proximal end of the housing, and said rod house being capable of being connected to a chamber house.

5 In yet another aspect the invention relates to a device for delivering a medicament or a diagnostic agent to the skin or mucosa of an animal, said device comprising

at least one rod house and at least one chamber house,

10 wherein the rod house comprises at least one housing, said at least one housing having a distal end and a proximal end, and at least one rod, said rod having a distal end and at least one proximal end, and said rod being slidably arranged in the housing, said rod being capable of being activated by being pushed towards the proximal end of the housing,

15 wherein the chamber house comprises at least one chamber, a first wall of said chamber being a first sealing and a second wall of said chamber being a second sealing, said first sealing and said second sealing being arranged so that an axis through said chamber may intersect both sealings, and said chamber comprising said medicament or said diagnostic agent, and

20

wherein the chamber house is provided with a labelling means for transferring a label to the animal being tested.

#### Drawings

25

Fig. 1 shows an assembled device according to the invention.

Fig. 2 shows a rod.

30

Fig. 3 shows the cap of the rod house.

Fig. 4 shows a locker bushing of the rod house.

Fig. 5 shows a proximal bushing of the rod house.

35

5

Fig. 6 shows a marking means.

Fig. 7 shows a chamber house.

5 Fig. 8 shows a plug.

Fig. 9 shows a pressing aid.

10 Fig. 10a, 10b, and 10c illustrate the different positions of the rod before, during and after activation.

Fig. 11a, 11b and 11c show one embodiment of a multidevice composed of ten single devices.

15 Fig. 12 shows another embodiment of a multidevice having three separate rod houses and one chamber house with three chambers.

#### Detailed description of the invention

20 The present invention relates to a device for delivering a medicament or a diagnostic agent to the skin or mucosa of an animal. In particular the device is suitable for allergy tests, wherein an amount of an allergen is delivered into the skin or mucosa of the animal to be tested and the animal's reaction to the allergen is monitored.

25 The animal may be any animal, in particular a mammal, such as a horse, a dog, and a cat; more specifically the mammal is a human being.

30 The device according to the invention comprises two separate components, namely at least one rod house and at least one separate chamber house, wherein said at least one chamber house is capable of being connected to the at least one rod house.

35 By constructing the device with two separate components the device fulfils several needs. First, during storage only the chamber house need cooled storage, since it is only the chamber house that comprises the allergen. Thereby the need for special-

ised storage has been reduced compared to prior art devices. Furthermore, the two components, rod house and chamber house, may be produced at separate locations, and need not be connected until immediately before use. This offers a great freedom in production logistics, since the allergen may be produced locally, and  
5 filled into the chamber house and subsequently assembled with the rod house.

#### Rod house

10 The rod house comprises at least one housing, wherein said at least one housing has a distal end and a proximal end, and at least one rod, and said rod has a distal end and at least one proximal end. Said rod is slidably arranged in the housing, whereby the term "slidably" means that the rod may be slid towards the proximal end of the housing. During use the rod is capable of being activated by being  
15 pushed towards the proximal end of the housing. In a preferred embodiment the rod is a longitudinal rod arranged axially in the rod house. By the longitudinal axial arrangement precision of the transfer of the medicament or diagnostic agent is increased, in that any play of the rod in the housing is reduced to a minimum.

20 The proximal of the rod house is preferably sealed by a rod house sealing. The sealing may be a stationary sealing to be penetrated by the needle during use, or a removable sealing, whereby the sealing is removed when the rod house is assembled with the chamber house. It is preferred that the sealing is stationary.

25 In a preferred embodiment the distal end of the rod is projecting out of the distal end of the rod house, whereby the rod may be activated by pressing the distal end of the rod towards the proximal end of the rod house. Preferably the rod house comprises means for retracting the rod after activation to ensure that the needle is retracted into the chamber house or rod house. The means for retracting the rod may be any suitable means, such as a spring or a pump. Preferably the means for retracting the  
30 rod is a spring.

35 To be able to predetermine how deep into the skin or mucosa of the individual the needle may travel, the housing preferably comprises stopper means for stopping advance of the rod at a predetermined position during activation, the stopper means may be any suitable means, such as a mechanical stopper means, such as wherein

7

the stopper means is a shoulder in the housing dimensioned to engage a shoulder on the rod.

5 The rod house is made from any suitable material, preferably a plastic material capable of being moulded, such as injection moulded. The rod house may be formed in one part or constructed from two or more parts assembled to form the rod house.

10 An example of materials selected for the rod house is polypropylene, such as a polypropylene having the following properties:

	Typical value	Unit	Test method
Tensile modulus	1300-1400	MPa	ISO 527-2
Tensile stress at yield	20-30	MPa	ISO 527-2
Tensile strain at yield	4-8	%	ISO 527-2
Rockwell hardness	80-90	R-scale	ISO 2039-2

In particular, the polypropylene is BC245MO from Borealis A/S, Denmark.

#### Needle

15

The proximal end of the rod is provided with means for transferring the medicament or the diagnostic agent to the animal. This is preferably arranged by providing the proximal end of the rod with a tapering end, either by integrating a needle in the proximal end or by forming the proximal end of the rod as a needle.

20

In order to ensure transfer of a sufficient amount of medicament or diagnostic agent, the proximal end of the rod is preferably provided with at least one recess.

25

The at least one recess may be arranged in any suitable part of the proximal end of the rod, such as in the tapering portion of the needle, the only requirement being the medicament or diagnostic agent in the recess is transferred to the animal during normal transfer. The recess may have its opening into the tip of the rod or into the longitudinal part of the rod.



8

In a preferred embodiment the proximal end of the rod is provided with more than one recess, such as at least two recesses, for example at least four recesses.

5 The rod material is preferably a material having a high strength. In particular when the needle is made from the same material as the rest of the rod.

Examples of materials for the rod are polypropylene, polypropylene mixed with glass fibre, polyamide metals and metal alloys, and mixtures thereof.

10 Since the needle penetrates two sealings before penetrating the skin, it is necessary that the needle maintains the shape and is not blunted during penetration of the sealings. Accordingly, in a preferred embodiment, the requirements to the needle material are at least the following mechanical properties:

	Typical value	Unit	Standard
Compressive strength	110-130	MPa	ASTM D695
Shear strength	50-70	MPa	ASTM D732
Taber abrasion, CS-17, 1 kg	20-25	mg/1000cy	GE
Tensile stress at break, 5 mm/min	110-140	MPa	ISO 527
Tensile strain at break, 5 mm/min	1.7-2.5	%	ISO 527
Tensile modulus, 1 mm/min	9000-11000	MPa	ISO 527
Flexural strength at break, 2 mm/min	200-250	MPa	ISO 178
Flexural modulus, 2 mm/min	9000-10000	MPa	ISO 178
Hardness, H358/30	100-130	MPa	ISO 2039/1
Hardness, Rockwell R	100-130	-	ISO 2039/2

15

In a preferred embodiment, the needle is made from Valox® from General Electric Plastics B.V., or from Miramid® H3KC, Plastcom A/S, Denmark.

20 In one aspect the invention relates to a rod house separate from a chamber house. The rod house is as described above. The separate rod house may be produced and sold separate from the chamber house for being connected before use.

### Chamber house

5 The chamber house comprises a chamber, wherein a first wall of said chamber is a first sealing and a second wall of said chamber is a second sealing, said first sealing and said second sealing are arranged so that an axis through said chamber may intersect both sealings, and said chamber comprising said medicament or said diagnostic agent.

10 As described above it is an advantage that the chamber house is separate from the rod house. During use the chamber house is either arranged adjacent the rod house or attached to the rod house. The chamber house is arranged in relation to the rod house so that the rod penetrates both sealings during use. Accordingly, the chamber house may be connected to the rod house so that the proximal end of the rod penetrates the first sealing and the second sealing when slid proximally.

15 In a preferred embodiment the chamber house has means for being attached to the rod house. The chamber house may be attached to the rod house either releasably or non-releasably by any suitable means. In one embodiment the distal part of the chamber house is provided with adhesive material, so that the chamber house and rod house are connected by means of the adhesive material. In another embodiment the chamber house and the rod house are connected through mechanical means, such as mechanical means selected from a thread, a luer lock, a bajonet lock, and a snap fit lock. In a preferred embodiment the chamber house are attached to the rod house through a snap fit lock.

25 The first sealing and the second sealing are attached to the chamber house by any suitable means. In one embodiment at least the first sealing is integrated with the walls of the chamber house.

30 In a preferred embodiment the second sealing is releasably attached to the chamber house, such as by means of a plug inserted into the chamber house. By closing the chamber of the chamber house with a plug the filling of the chamber is facilitated. After sealing the chamber with the plug the medicament or diagnostic agent is enclosed in the chamber reducing the risk of atomizing of the medicament or diagnostic agent thereby reducing the risk of contamination of the environment.

35

The chamber house may be formed from any suitable material, capable of being produced in a cost effective manner. Furthermore, the chamber house material must not react with the medicament or diagnostic agent.

5

10

Preferably the chamber house is made from a plastic material, more preferably from a resilient material. In particular when the chamber house is attached to the rod house by means of a snap fit lock it is desired that the material is resilient. Furthermore, the resilient material offers a more pleasant feeling to the individual being tested when the chamber house is arranged on the skin or mucosa. Also the sealings are preferably produced from a resilient plastic material. If the chamber house is produced from a harder material than the sealing, the chamber house may be produced for example by two-component moulding.

15

Examples of the chamber house material are a thermoplastic material, such as a rubber, a polyolefin or mixtures thereof, in particular a plastic material having the following characteristics:

	Typical value	Unit	Standard
Hardness	35-50	Shore A	ASTM D2240
Density	0.9-1.1	g/cm <sup>3</sup>	ASTM D792
Tensile strength	3.0-5.0	MPa	ASTM D638
E-100	0.5-0.7	MPa	ASTM D638
E-300	1.3-1.8	MPa	ASTM D638
Elongation at break	500-600	%	ASTM D638
Tear strength	12-20	kN/m	ASTM D624

20

In particular, the chamber house material may be Dryflex® from Nolato Elastoteknik AB, Sweden.

25

25

The plug may be made from the same material as the chamber house or from another material, preferably a thermoplastic material. In particular the plug may be made from a natural or synthetic rubber, such as a material having the following characteristics:

	Typical value	Unit	Standard
Hardness	94	Shore A	DIN 53505
Density	1.13	g/cm <sup>3</sup>	DIN 53479
Tensile strength	14.5	N/mm <sup>2</sup>	DIN 53504
Elongation at break	610	%	DIN 53504
Modulus at 100%	6.0	N/mm <sup>2</sup>	DIN 53504
Modulus at 200%	6.6	N/mm <sup>2</sup>	DIN 53504
Modulus at 300%	7.5	N/mm <sup>2</sup>	DIN 53504

Most preferably, the plug is made from Thermoplast K TF9AAE from Kraiburg TPE GmbH, Germany.

5 In one aspect, the invention relates to a chamber house for being connected to a rod house as defined above, wherein the chamber house is as defined above. The chamber house may be sold separate from the rod house for being connected immediately before use. The at least one chamber may be prefilled at least partly with medicament or diagnostic agent, such as prefilled with an allergen or a combination of allergens.

10 In another embodiment the chamber house is sold empty to be filled with medicament or diagnostic agent locally before use. This is especially relevant when using with allergens of only local relevance.

#### 15 Marking means

To increase the security of the device, it is preferably provided with marking means to mark that the rod has been activated, whereby accidental re-use of the device is avoided. The marking means may be any suitable means such as change of physical appearance in at least a part of the device, such as change of colour and/or change of shape.

25 In a preferred embodiment the marking means is a marker projecting from the distal end of the housing and said marking means is activated when the rod is activated. For example the at least one marking means is a marker being arranged concentrically around at least a part of the distal end of the rod. Thereby the marking means

## 12

is pressed forwards towards the proximal end of the device when the rod is activated. Furthermore, it is preferred that once the marker means has been activated it takes a new position or changes colour. For example in one embodiment the housing comprises means for engaging the marker means when the marker means is activated, thereby holding the marker means in a new position after activation.

The marking means may be made from any suitable material; however it is preferred that the marker means has a colour different from the colour of the distal end of the rod.

### Multidevice

The device according to the invention may be a device constructed to transfer one type of medicament or diagnostic agent. However, in another embodiment the device according to the invention may be a multidevice or part of a multidevice, wherein the term multidevice means a device comprising two or more different medicaments and/or diagnostic agents.

In particular when the device is used for transfer of diagnostic agents, such as allergens in an allergy testing, a series of different allergens is normally used. Thus, it is advantageous to arrange the device as a multidevice having the number of chambers with medicament or diagnostic agent corresponding to the number of different medicaments or diagnostic agents in the series, whereby all medicaments or diagnostic agents may be transferred at once. Furthermore, a multidevice may secure the order in which the medicament or diagnostic agent is transferred.

A multidevice may be constructed by arranging two or more chamber houses as described above, as well as either two or more rods, or a rod with two or more needles capable of transferring the medicament and/or diagnostic agent from the two or more chambers. In order to assure the security of the device, it must be assured that a needle only transfers one medicament or diagnostic agent, to avoid mixing of medicaments or diagnostic agents.

In one embodiment the device comprises at least two chamber houses, such as at least three chamber houses. The chamber houses may be separate from each

other; however in a preferred embodiment the at least two chamber houses are connected.

5 In one embodiment, with respect to a multidevice, the rod has at least two proximal ends, such as at least three proximal ends. Such a rod having more than one proximal end, may be have one common distal end.

10 In another embodiment the rod house comprises the same number of rods as the number of chambers. Thus, in one embodiment the rod house comprises at least two rods, such as at least three rods.

15 When a multidevice comprises two or more rods, it may be advantageous to apply a common activation means to the rods, for example to be able to activate all rods in one operation. Accordingly, in one embodiment two or more rods are connected at their distal ends to a common activation means, such as a connector cap.

#### Labelling means

20 The device according to the invention is in one embodiment provided with a labelling means, so that the skin or the mucosa of said mammal is labelled when the medicament or diagnostic agent is delivered to the mammal. The labelling means may be applied to the skin or mucosa before, during or after transfer of the medicament or diagnostic agent.

25 The labelling means may be any suitable labelling, such as a tape or a colour or letters or figures, or a combination thereof, such as a code identifying the content of the chamber and/or the individual being tested. The labelling means is preferably arranged on the chamber house, so that it is transferred during use of the device, for example by a stamping effect when the labelling means is arranged on the proximal  
30 part of the chamber house.

#### Use

35 The device according to the invention is suitable for delivering a medicament or a diagnostic agent to the skin or mucosa of an animal, such as a human being.

Accordingly, one aspect of the invention relates to a method for delivering a sufficient amount of medicament or diagnostic agent to a mammal in need thereof, comprising

5

- arranging a device as defined above, wherein the chamber house comprising the medicament or diagnostic agent is connected to the rod house, adjacent the skin or mucosa of said animal,

10

- activating the rod of the device, thereby delivering said medicament or diagnostic agent to said animal.

The device and method is suitable for delivering any kind of medicament or diagnostic agent to the skin or mucosa of the animal.

15

In relation to medicaments, the invention in particular relates to delivery of vaccines, probiotics, antibiotics or vitamins, preferably to delivery of vaccines.

20

In relation to diagnostic agents, the invention in particular relates to delivery of allergens for allergy tests. In this relation the chamber house comprises an allergen or combination of allergens.

25

In one embodiment the devices are used singly for delivering the determined medicaments or diagnostic agents, it is however preferred when delivering allergens that the device is arranged as a multidevice for delivering the series of allergens necessary for the testing in one application round.

30

The allergens used may be any allergens used for testing for allergy, such as pollen from various plants, moulds, insect venoms, food allergens, house dust mite allergens, and animal hair. In relation to individuals to be treated in a hospital it may be necessary to test for latex allergy. In particular when treating unconscious individuals before for example an operation. For latex allergy test a multidevice comprising three chambers is suitably used, wherein one chamber comprises latex allergen, one chamber comprises saline, and one chamber comprises histamin, the latter two

15

being negative and positive controls, respectively. For latex allergy tests the three chambers are preferably arranged in chamber houses being connected.

**Reference signs in drawings**

5

1 Device according to the invention

2 Housing

3 Chamber house

4 Chamber

10

5 Marker means

6 Cap

7 Spring

8 Plug

9 Projecting means

15

10 Projecting means on marker means

11 Bushing

12 Distal end of rod

13 Needle

14 Shoulder on rod

20

15 Internal bushing

16 Opening

17 Recess in chamber house

18 First sealing

19 Recess for receiving a plug

25

20 Recess for receiving distal end of the rod

21 Connector

22 Bracelet

23 Opening for receiving a device according to the invention

24 Recess for receiving bracelet

30

25 Connector cap

26 Package with three devices according to the invention

27 Holder

28 Connector cap

29 Rod

35

30 Recess in tip of rod



16

- 31 Rib on housing
- 32 Projecting part on bushing
- 33 Second sealing
- 34 Stem

5

#### Detailed description of the invention in relation to the drawings

In the following one embodiment of the invention is described in relation to the drawings.

10

In Fig. 1 a device 1 according to the invention is shown. The device 1 is assembled of a rod house comprising a housing 2 and a rod 29, and a chamber house 3 comprising chamber 4. In the shown embodiment the rod house consists of housing 2, an internal bushing 15, and a bushing 11. The rod house further encloses rod 29 arranged axially in the housing 2, spring 7 arranged concentrically around rod 29, as well as marker means 5 arranged concentrically around the distal end 12 of the rod 29. Furthermore, the distal end of the rod 29 is provided with a cap 6 facilitating the activation of the rod 29. In the proximal end of the device 1 the chamber house 4 is connected to the rod house through a snap fit lock to the bushing 11. The chamber house 3 is provided with a plug 8, defining a chamber 4 between one wall of the chamber house 3 and the plug 8.

20

In Fig. 2 the rod 29 is shown in greater detail. The proximal end of the rod 29 is provided with a tip 13 having at least one recess 30. In Fig. 2b the tip is seen from the proximal end of the rod, showing 4 recesses 30. The rod 29 is furthermore provided with a shoulder 14 capable of functioning as a stopper means controlling the advancing movement of the rod 29, when the rod 29 is activated.

25

In Fig. 3, the housing 2 is shown in greater detail. The housing 2 is preferably provided with ribs 31 for a better grip of the device 1.

30

In Fig. 4 the internal bushing 15 is shown in greater detail. Projecting means 9 is arranged to engage the marker means when the rod 29 is activated.

## 17

In Fig. 5 the bushing 11 is shown in greater detail. The bushing 11 is arranged in the proximal end of the housing 2 in the device 1 projecting from the proximal end. The rod 29 is capable of sliding through opening 16 of bushing 11. Furthermore, bushing 11 is provided with a projecting part 32 capable of engaging the chamber house 3 when the chamber house 3 and the rod house are connected in a snap fit lock.

In Fig. 6 the marker means 5 is shown in greater detail. The marker means is provided with a central bore for receiving the rod 29, when assembled. The marker means is also provided with a projecting part 10 capable of engaging the projecting means 9 on the internal bushing 15.

In Fig. 7, the chamber house 3 is shown in greater detail. The chamber house 3 comprises recess 17 capable of housing the proximal part of bushing 11 when the chamber house 3 is connected to the rod house. Furthermore, the chamber house 3 comprises a first sealing 18 as well as chamber 4. Recess 19 is arranged to receive a plug for providing the chamber house 3 with a second sealing. Plug 8 is shown in Fig. 8 having second sealing 33, whereby the plug 8 when inserted into the chamber house 3 encloses the chamber 4.

The cap 6 is shown in Fig. 9, wherein the recess 20 is capable of receiving the distal end of the rod 12.

In Fig. 10 the travelling of the rod before, during and after activation is shown. In Fig. 10a the rod 29 is positioned in its inactivated position. The marker means 5 is located around the distal end of the rod and projects from the distal end of the rod house. The cap 6 is arranged on the distal end of the rod 29. The spring 7 is relaxed in the rod house. The tip 13 of the rod is positioned in the bushing 11, and the chamber 4 is filled with medicament or diagnostic agent. During activation of the rod 29, the rod 29 advances towards the proximal end of the device 1, penetrates the sealings of the chamber 4 and projects from the proximal end of the chamber house transferring medicament or diagnostic agent in its tip recesses. The marker means 5 is pressed into the housing 2 whereby projecting part 10 engages projecting means 9 of the housing. After activation the spring 7 forces the rod 29 backwards towards the distal end of the device 1 thereby the tip of the rod 29 is retracted into the chamber

18

house 3. The marker means 5 is maintained engaged in the rod house, thereby signalling that the rod 29 has been activated and should not be used anymore.

5 In Fig. 11a, a multidevice according to the invention is shown. The multidevice comprises 10 devices 1 being arranged in a connector 21. Each device 1 is position perpendicular to the connector 21. The distal end 12 of the rod of the device is projecting from the connector 21. The connector 21 may be fastened to the animal to be tested by means of a bracelet 22. In Fig. 11b the opening for receiving a device 1 in the connector 21 is shown. Furthermore, the connector 21 is provided with recess 10 24 for receiving a bracelet 22.

In Fig. 11c the multidevice of Fig. 11a is shown having a connector cap 25 arranged above each and every distal end of the rods, so that all rods may be activated by activating the connector cap 25.

15

In Fig. 12a a package of a multidevice comprising 3 devices 1 is shown. The 3 devices 1 are connected through a holder 27 and a connector cap 28, wherein the holder 27 and the connector cap 28 are connected by means of stem 34 which is shown in Fig. 12b.. The 3 chamber houses 3 are also connected, whereby the 20 chamber houses 3 may be provided as one unit.

**Claims**

1. A device for delivering a medicament or a diagnostic agent to the skin or mu-  
cosa of an animal, said device comprising
- 5 at least one rod house and at least one separate chamber house, wherein said  
chamber house is capable of being connected to the rod house,
- 10 wherein the rod house comprises at least one housing, said at least one housing  
having a distal end and a proximal end, and at least one rod, said rod having a  
distal end and at least one proximal end, and said rod being slidably arranged in  
the housing, said rod being capable of being activated by being pushed towards  
the proximal end of the housing, and
- 15 wherein the chamber house comprises at least one chamber, a first wall of said  
chamber being a first sealing and a second wall of said chamber being a second  
sealing, said first sealing and said second sealing being arranged so that an axis  
through said chamber may intersect both sealings, and said chamber comprising  
said medicament or said diagnostic agent.
- 20
2. The device according to claim 1, wherein the rod is a longitudinal rod arranged  
axially in the rod house.
- 25
3. The device according to claim 1 or 2, wherein the rod house is sealed by a re-  
movable rod house sealing in the proximal end.
4. The device according to any of the preceding claims, wherein the distal end of  
the rod is projecting out of the distal end of the rod house.
- 30
5. The device according to any of the preceding claims, wherein the proximal end  
of the rod is a needle having a tapering end.
6. The device according to any of the preceding claims, wherein the needle com-  
prises at least one recess in the tapering portion of the needle, such as at least

20

two recesses in the tapering portion of the needle, such as at least four recesses in the tapering portion of the needle,

- 5
7. The device according to any of the preceding claims, wherein the chamber house is connected to the rod house so that the proximal end of the rod penetrates the first sealing and the second sealing when slid proximally.
- 10
8. The device according to any of the preceding claims, wherein at least one marking means is arranged in the rod house to mark that the rod has been activated.
- 15
9. The device according to any of the preceding claims, wherein the at least one marking means is a marker projecting from the distal end of the housing and said marking means is activated when the rod is activated.
- 20
10. The device according to any of the preceding claims, wherein the at least one marking means is a marker being arranged concentrically around at least a part of the distal end of the rod.
- 25
11. The device according to any of the preceding claims, wherein the marking means is coloured in a colour different from the colour of the distal end of the rod.
- 30
12. The device according to any of the preceding claims, wherein the housing comprises means for engaging the marker means when the marker means is activated.
13. The device according to any of the preceding claims, wherein means for retracting the rod after activation is arranged in the housing.
14. The device according to any of the preceding claims, wherein the means for retracting the rod is a spring.

15. The device according to any of the preceding claims, wherein the housing comprises stopper means for stopping advance of the rod at a predetermined position during activation.
- 5 16. The device according to claim 15, wherein the rod has a shoulder and the stopper means is a shoulder in the housing dimensioned to engage the shoulder on the rod.
- 10 17. The device according to any of the preceding claims, wherein the chamber house has means for being attached to the rod house.
18. The device according to any of the preceding claims, wherein the second sealing is releasably attached to the chamber house.
- 15 19. The device according to any of the preceding claims, wherein the chamber house is made from a plastic material.
- 20 20. The device according to any of the preceding claims, wherein the chamber house is made from a resilient material.
21. The device according to any of the preceding claims, wherein the chamber house is attachable to the rod house by means of a thread or snap fit lock.
- 25 22. The device according to any of the preceding claims, wherein the rod has at least two proximal ends, such as at least three proximal ends.
23. The device according to any of the preceding claims, wherein the rod house comprises at least two rods, such as at least three rods.
- 30 24. The device according to claim 23, wherein the rods are connected at their distal ends to a common activation means.
- 35 25. The device according to any of the preceding claims, wherein the device comprises at least two chamber houses, such as at least three chamber houses.

22

26. The device according to claim 25, wherein at least two chamber houses are connected.

5 27. The device according to any of the preceding claims, wherein the device is provided with a labelling means, so that the skin or the mucosa of said animal is labelled when the medicament or diagnostic agent is delivered to the animal.

10 28. The device according to any of the preceding claims, wherein the labelling means is arranged on the chamber house.

29. The device according to any of the preceding claims, wherein the at least one chamber is filled at least partly with medicament or diagnostic agent.

15 30. A method for delivering a sufficient amount of medicament or diagnostic agent to an animal in need thereof, comprising

- 20 - arranging a device as defined in any of the claims 1-29, wherein the chamber house comprising the medicament or diagnostic agent is connected to the rod house, adjacent the skin or mucosa of said animal,
- activating the rod of the device, thereby delivering said medicament or diagnostic agent to said animal.

25 31. The method according to claim 30, wherein the chamber house comprises an allergen or combination of allergens.

30 32. A chamber house for being connected to a rod house as defined in any of claims 1-29, wherein the chamber house comprises a chamber, a first wall of said chamber being a first sealing and a second wall of said chamber being a second sealing, said first sealing and said second sealing being arranged so that an axis through said chamber may intersect both sealings, and said chamber comprising a medicament or a diagnostic agent.

35 33. The chamber house according to claim 32, wherein the chamber is at least partly filled with an allergen or a combination of allergens.

34. A rod house comprising at least one housing, said at least one housing having a distal end and a proximal end, and at least one rod, said rod having a distal end and at least one proximal end, and said rod being slidably arranged in the housing, said rod being capable of being activated by being pushed towards the proximal end of the housing, and said rod house being capable of being connected to a chamber house as defined in any of the claims 1-29.
35. A device for delivering a medicament or a diagnostic agent to the skin or mucosa of an animal, said device comprising
- at least one rod house and at least one chamber house,
- wherein the rod house comprises at least one housing, said at least one housing having a distal end and a proximal end, and at least one rod, said rod having a distal end and at least one proximal end, and said rod being slidably arranged in the housing, said rod being capable of being activated by being pushed towards the proximal end of the housing,
- wherein the chamber house comprises at least one chamber, a first wall of said chamber being a first sealing and a second wall of said chamber being a second sealing, said first sealing and said second sealing being arranged so that an axis through said chamber may intersect both sealings, and said chamber comprising said medicament or said diagnostic agent, and
- wherein the chamber house is provided with a labelling means for transferring a label to the animal being tested.
36. The device according to claim 35, wherein the device has one or more of the features of claims 1-29.



1/14

Modtaget

30 MAJ 2003

PVS

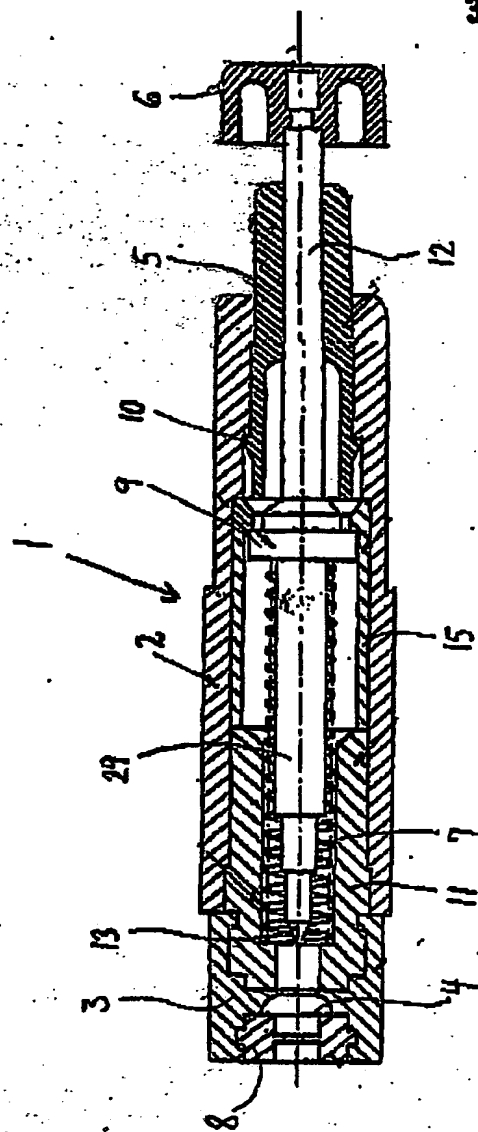


Fig. 1


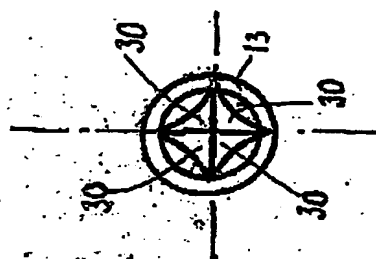


Fig. 2b

2/14

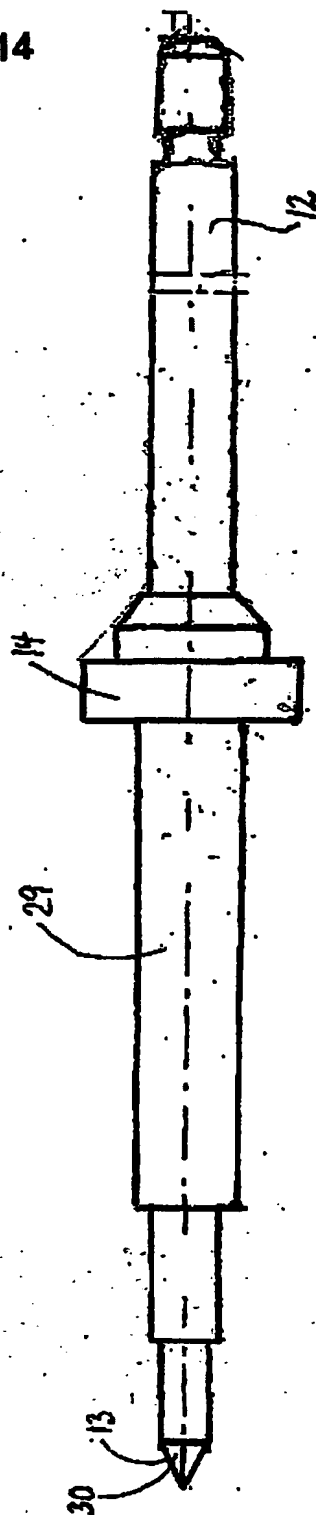

Modtaget  
30 MAJ 2003  
PVS

Fig. 2a

3/14

Modtaget

30 MAJ 2003

PVS

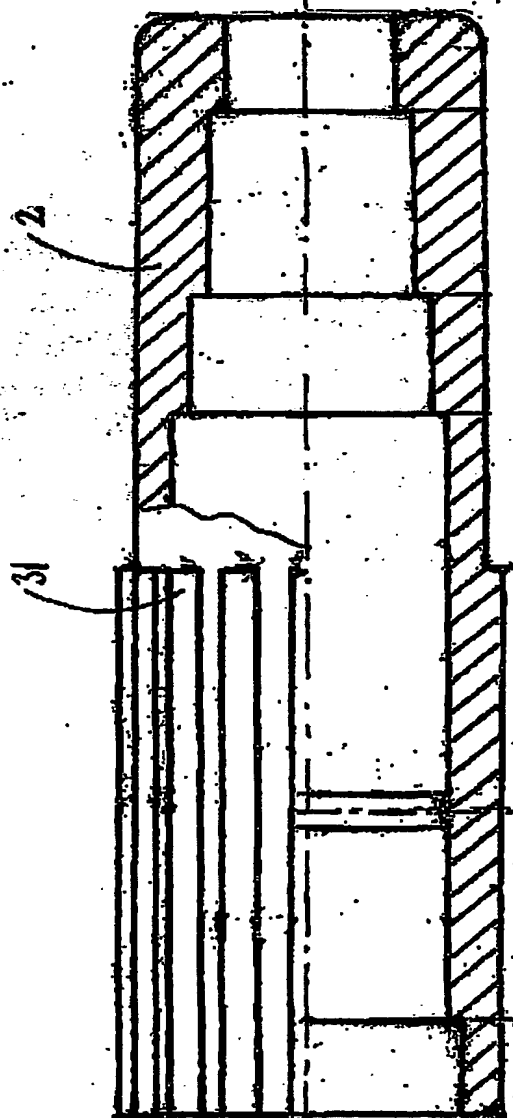


Fig. 3




4/14

Modtaget

30 MAJ 2003

PVS

Fig. 4

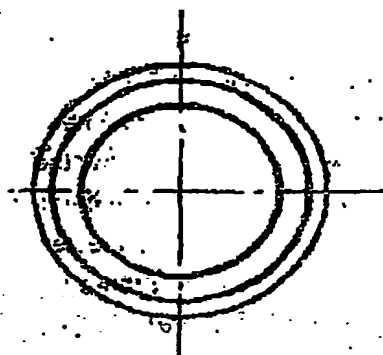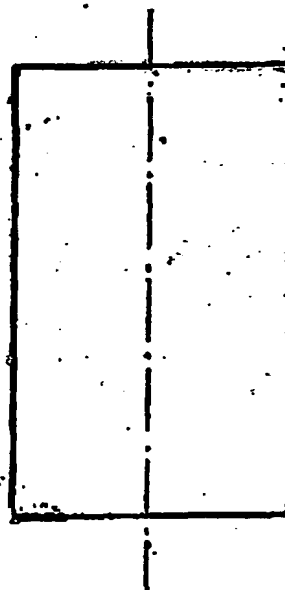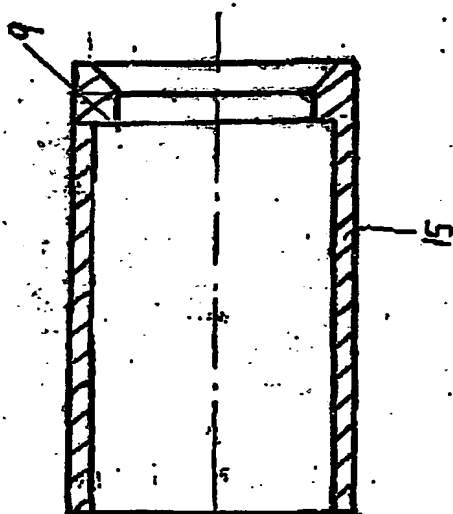


5/14

Modtaget

30 MAJ 2003

PVS

**Fig. 5**

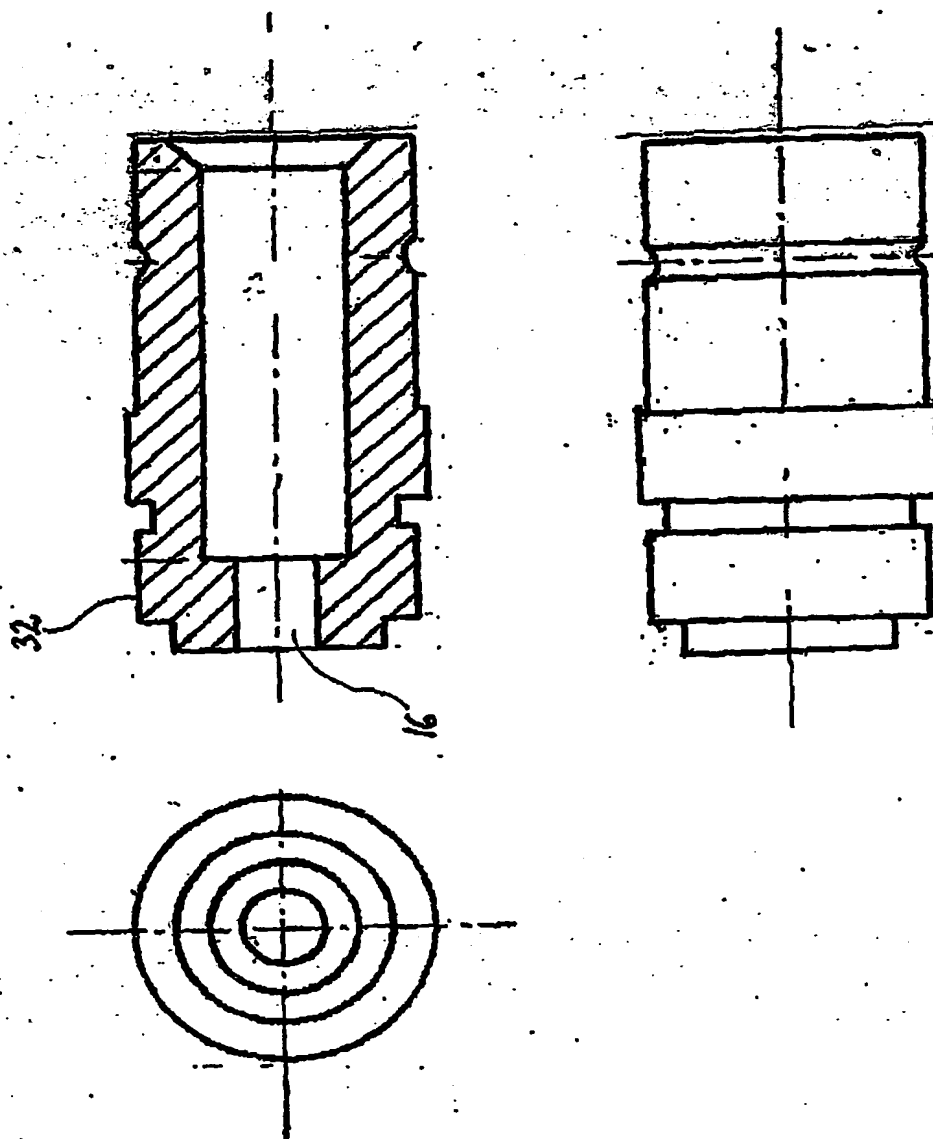


6/14

Modtaget

30 MAJ 2003

PVS

**Fig. 6**

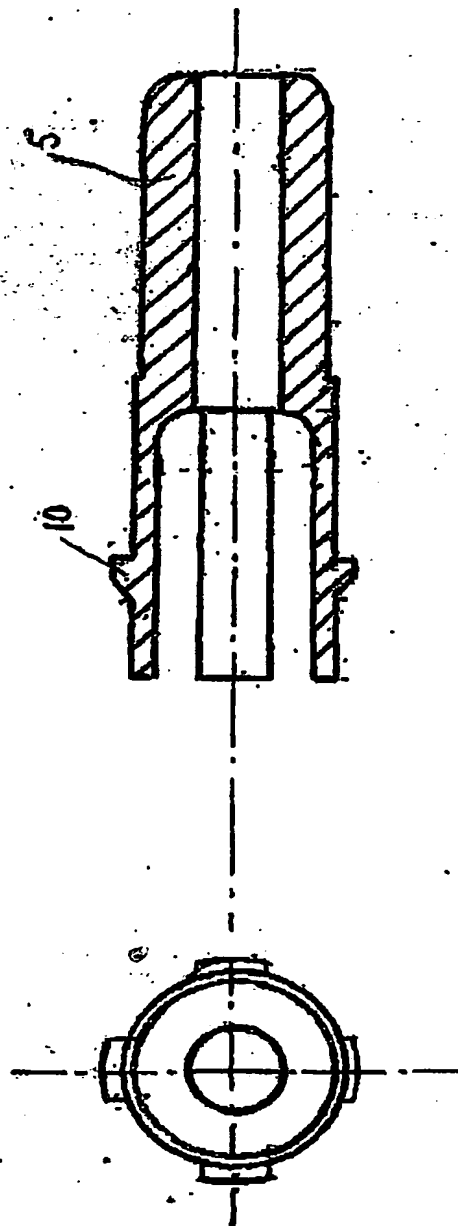



7/14

Modtaget

30 MAJ 2003

PVS

**Fig. 7**

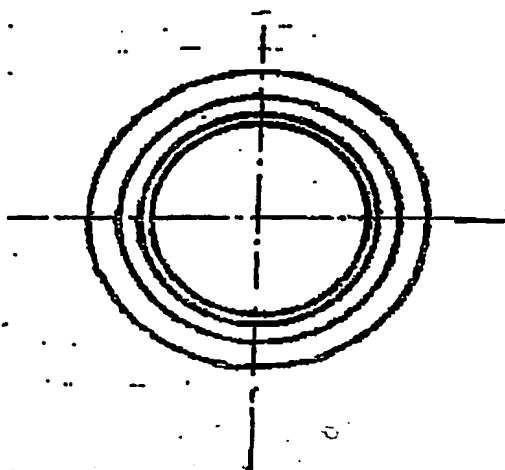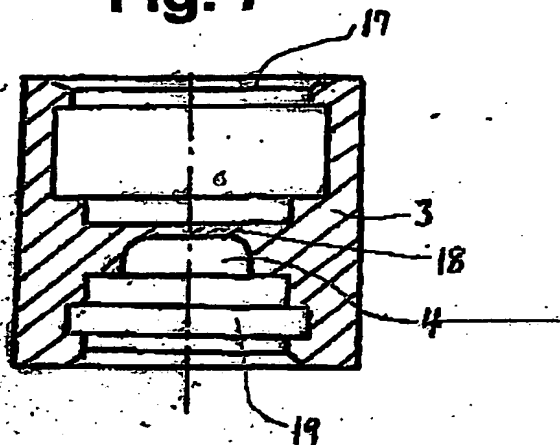

0/05 2003 16:16 FAX 33320384

HOIBERG A/S

PVS

033/038



8/14

Modtaget

30 MAJ 2003

PVS

Fig. 8

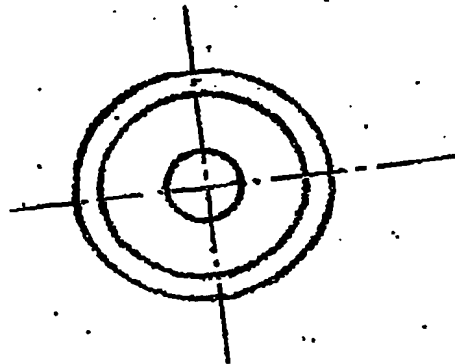




9/14

**Fig. 9**

Modtaget

30 MAJ 2003

PVS

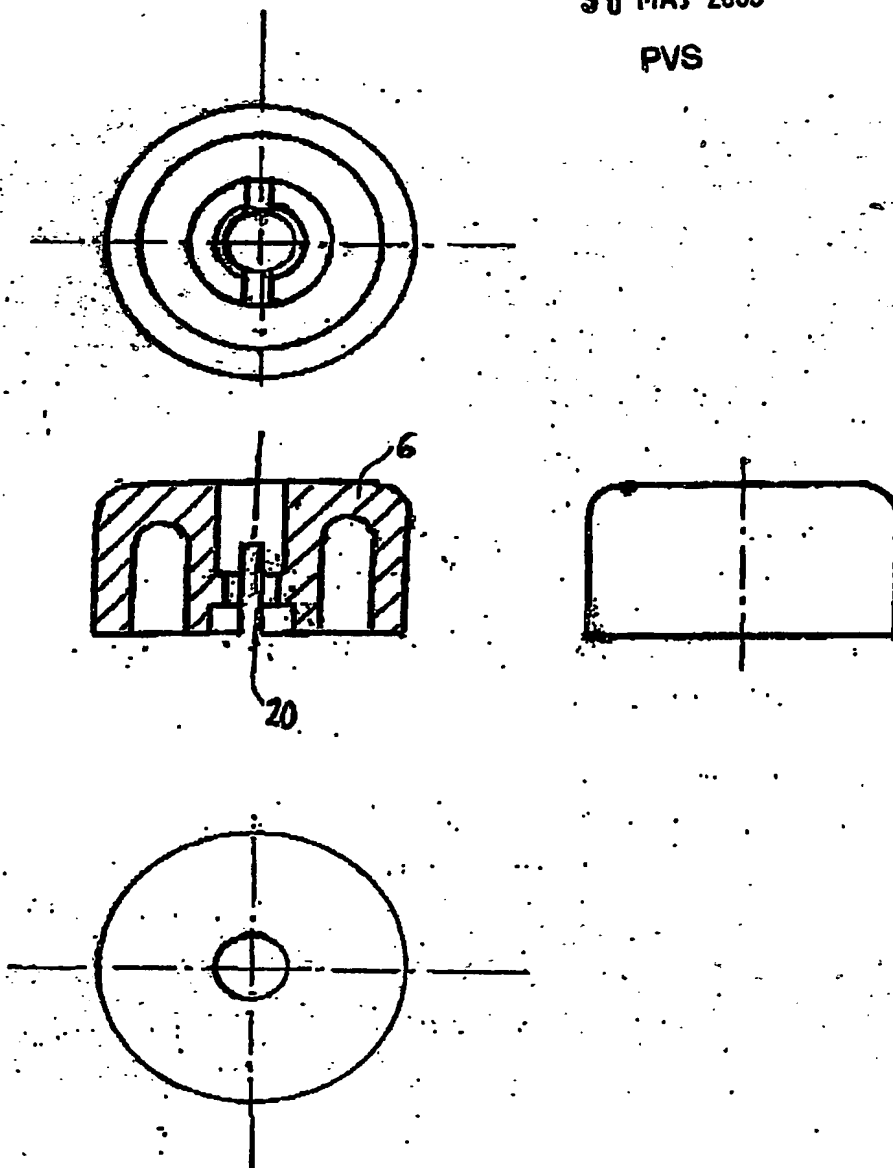


10/14

Modtaget

30 MAJ 2003

PVS

**Fig. 10**

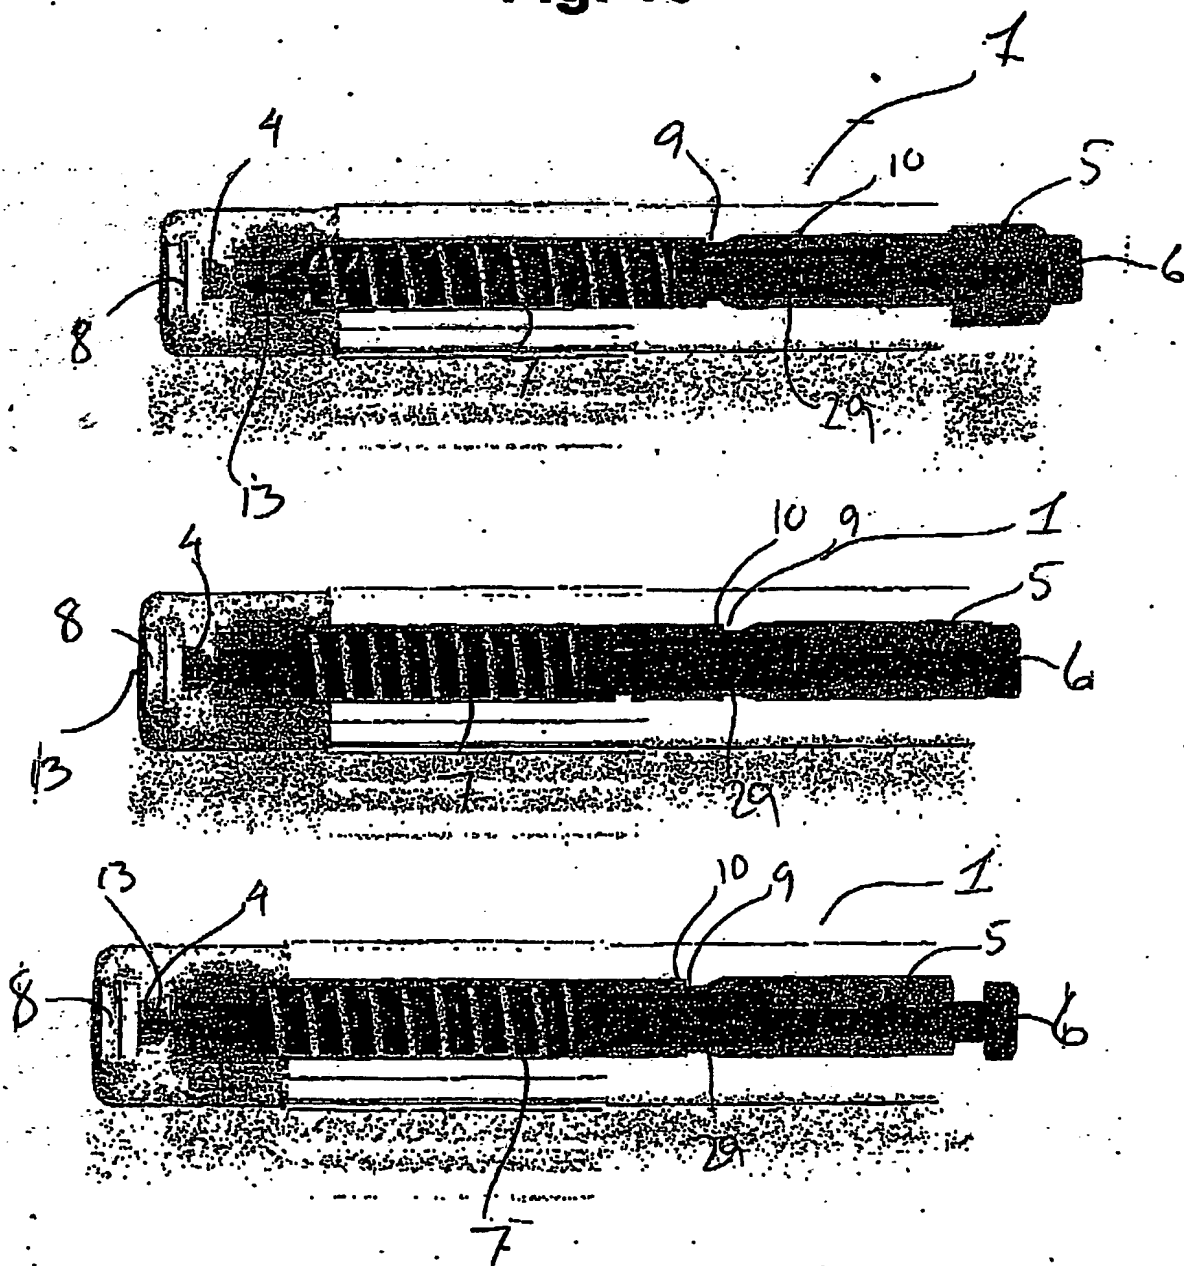

11/14

Modtaget

30 MAJ 2003

• PVS

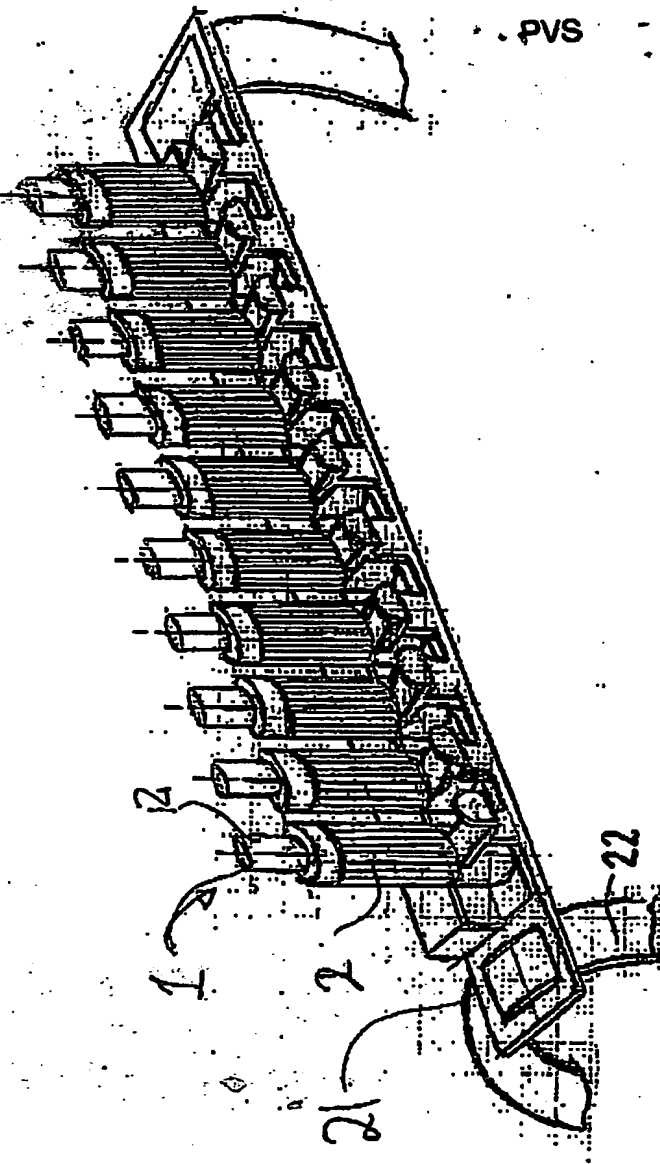


Fig. 11a

12/14

Modtaget

30 MAJ 2003

PVS

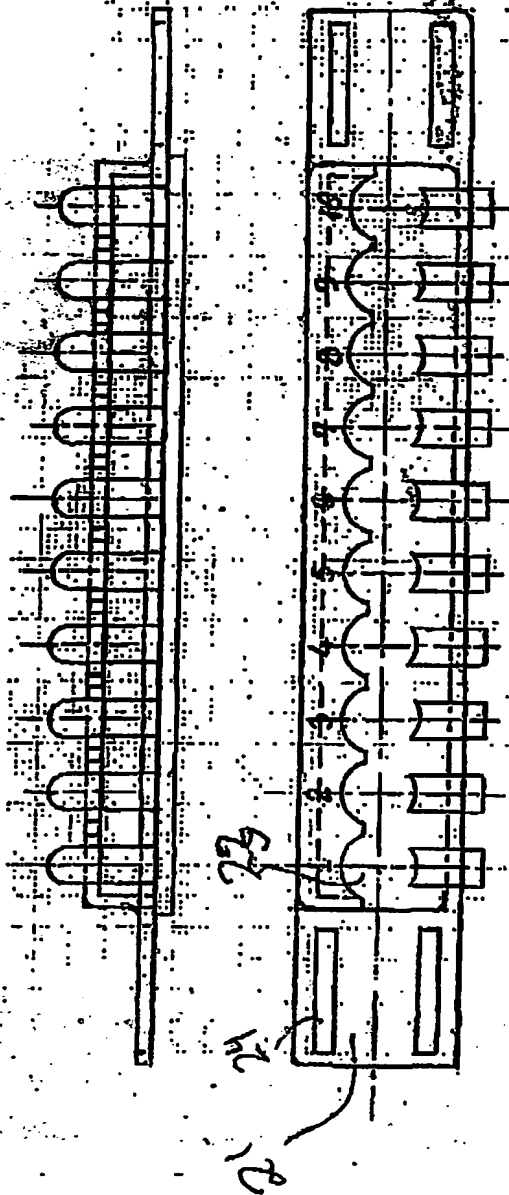


Fig. 11b


13/14

Modtaget

30 MAJ 2003

**Fig. 11c**

PVS

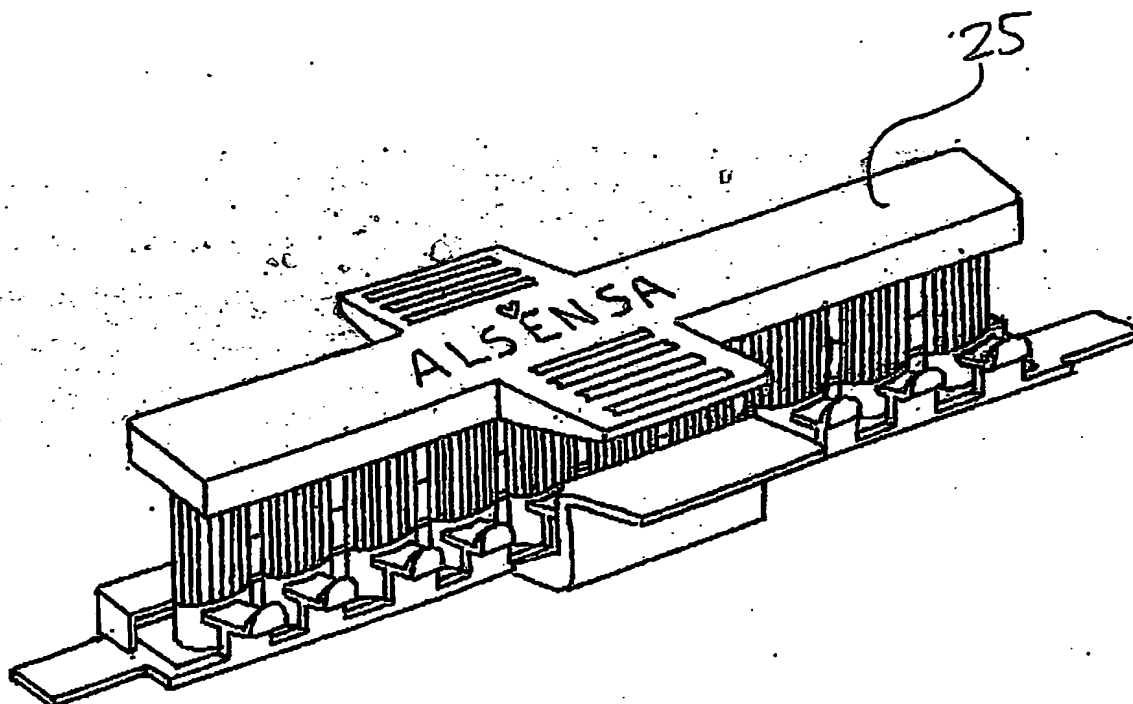

14/14

Modtaget

30 MAJ 2003

PVS

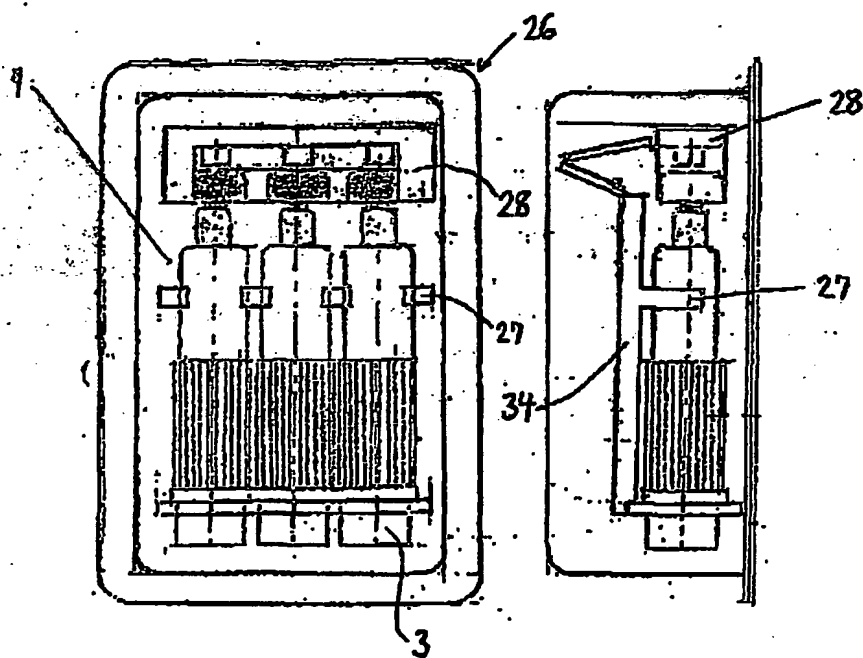


Fig. 12a

Fig. 12b

This Page is inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record

## BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☒ BLURED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☐ COLORED OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☒ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☒ REPERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images  
problems checked, please do not report the  
problems to the IFW Image Problem Mailbox**